

1/6


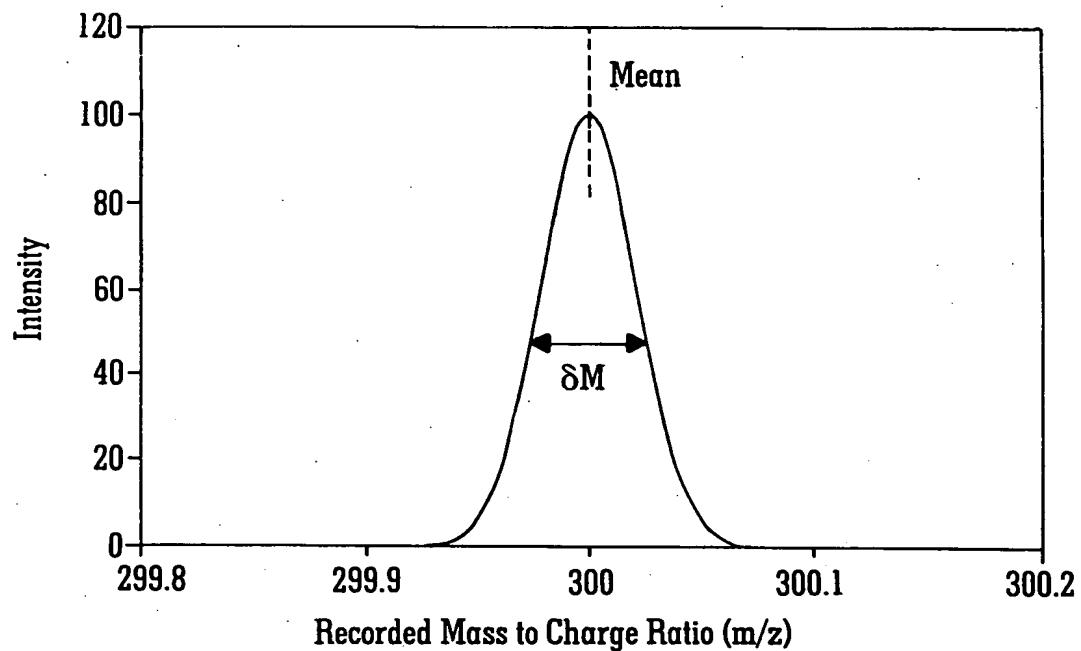


FIG. 1

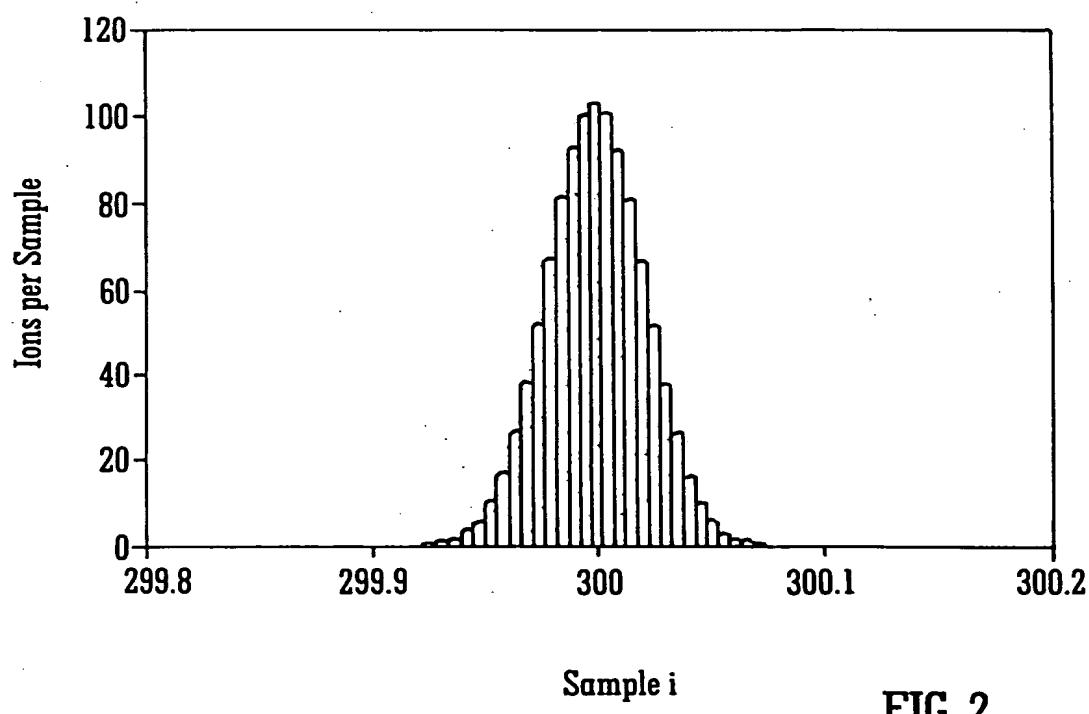

Sample i

FIG. 2

2/6

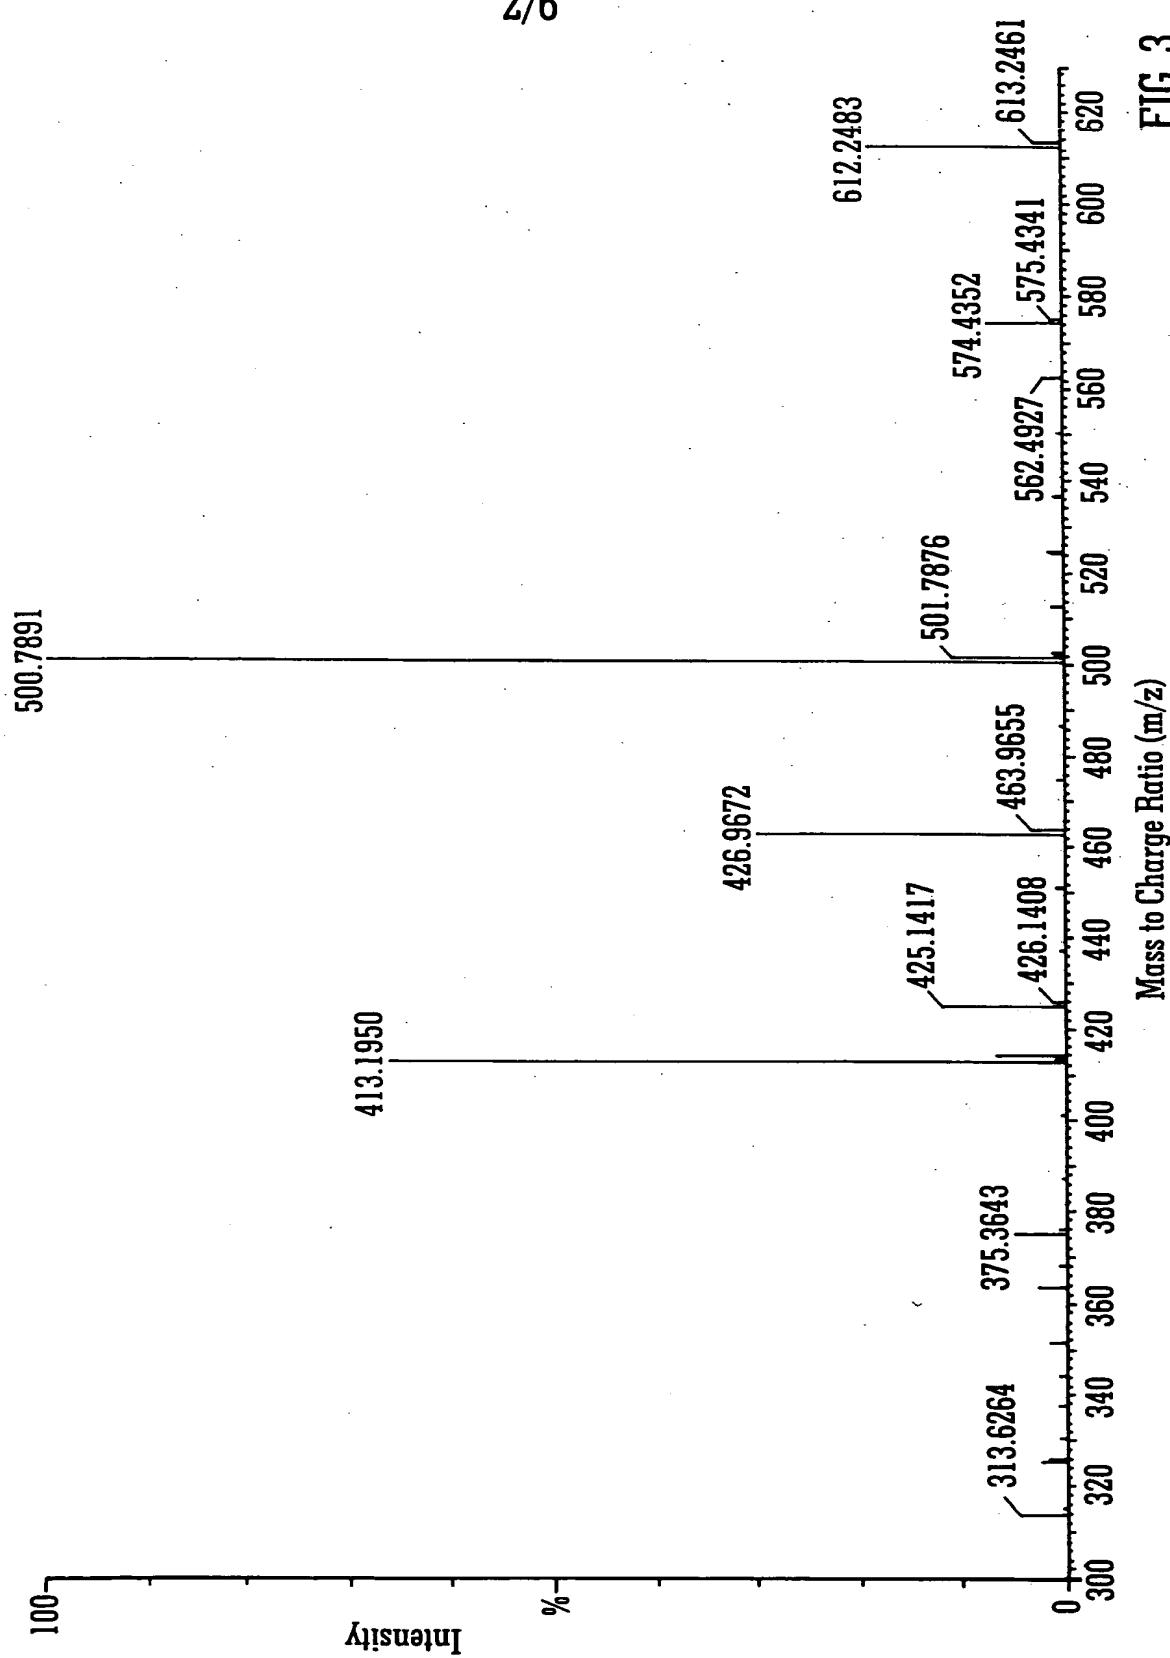


FIG. 3

3/6

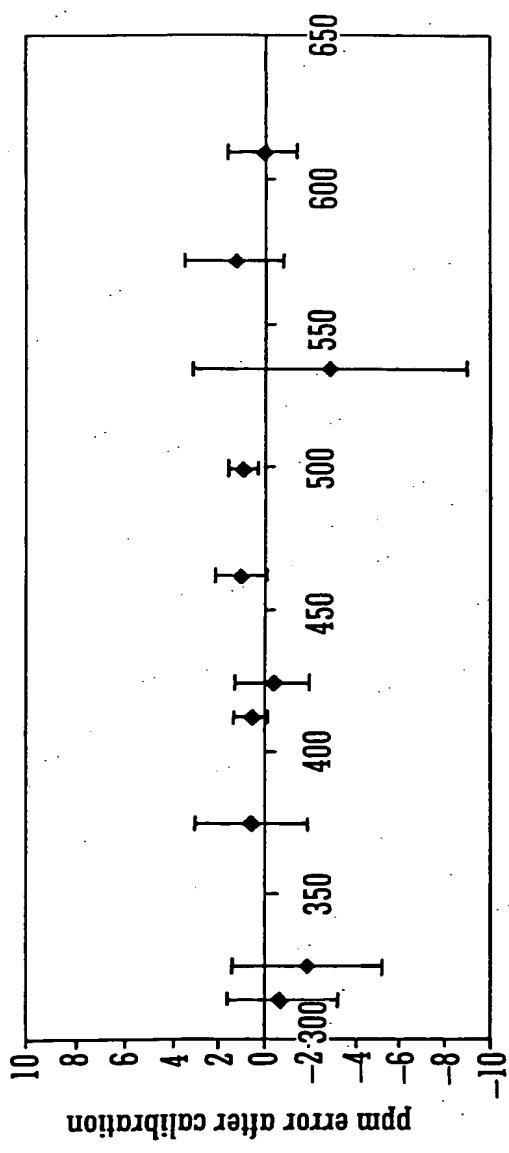


FIG. 4
Calibration Reference m/z

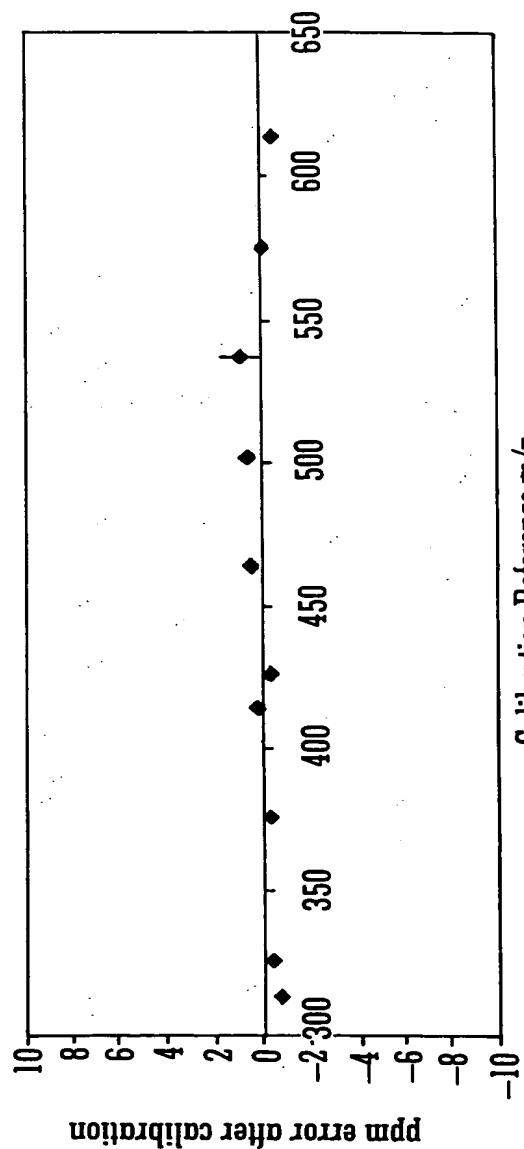


FIG. 5
Calibration Reference m/z

4/6

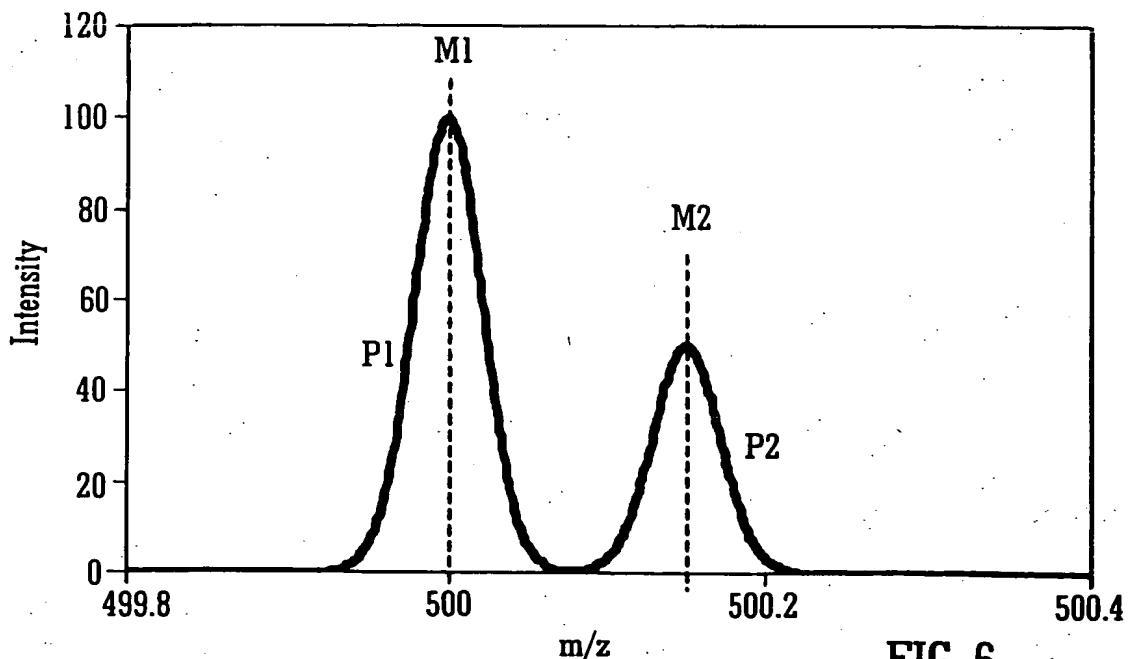


FIG. 6

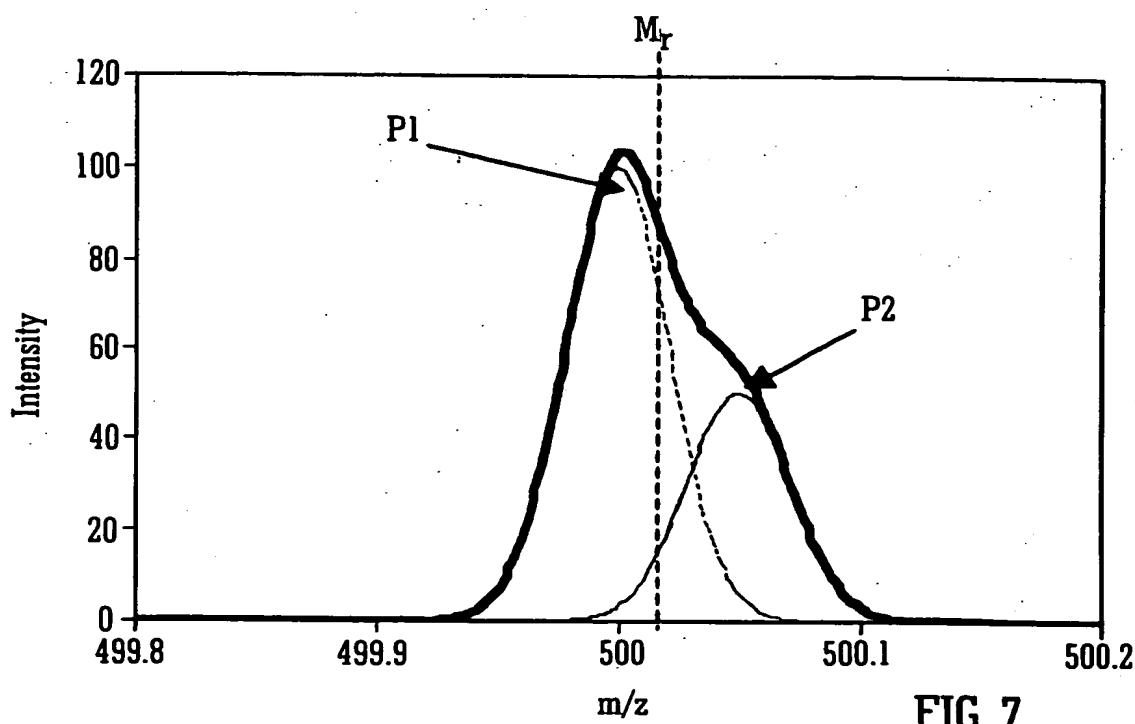


FIG. 7

5/6

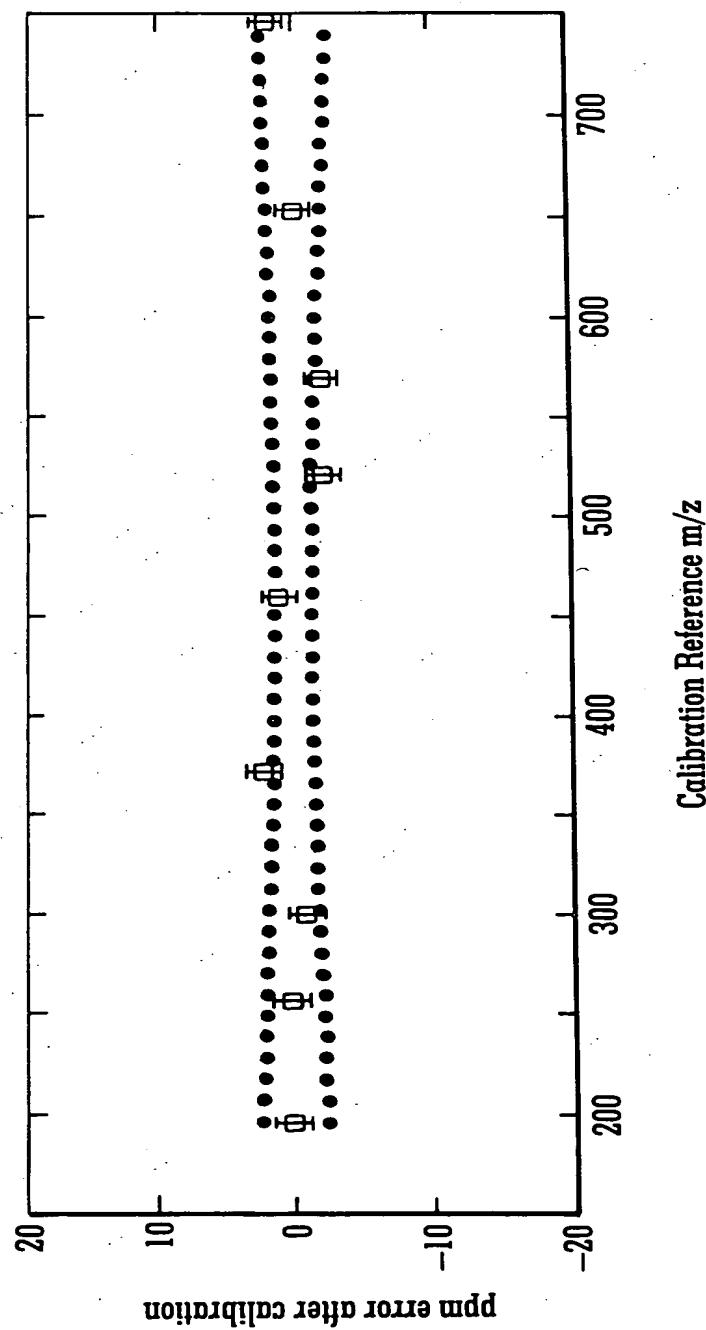


FIG. 8

6/6

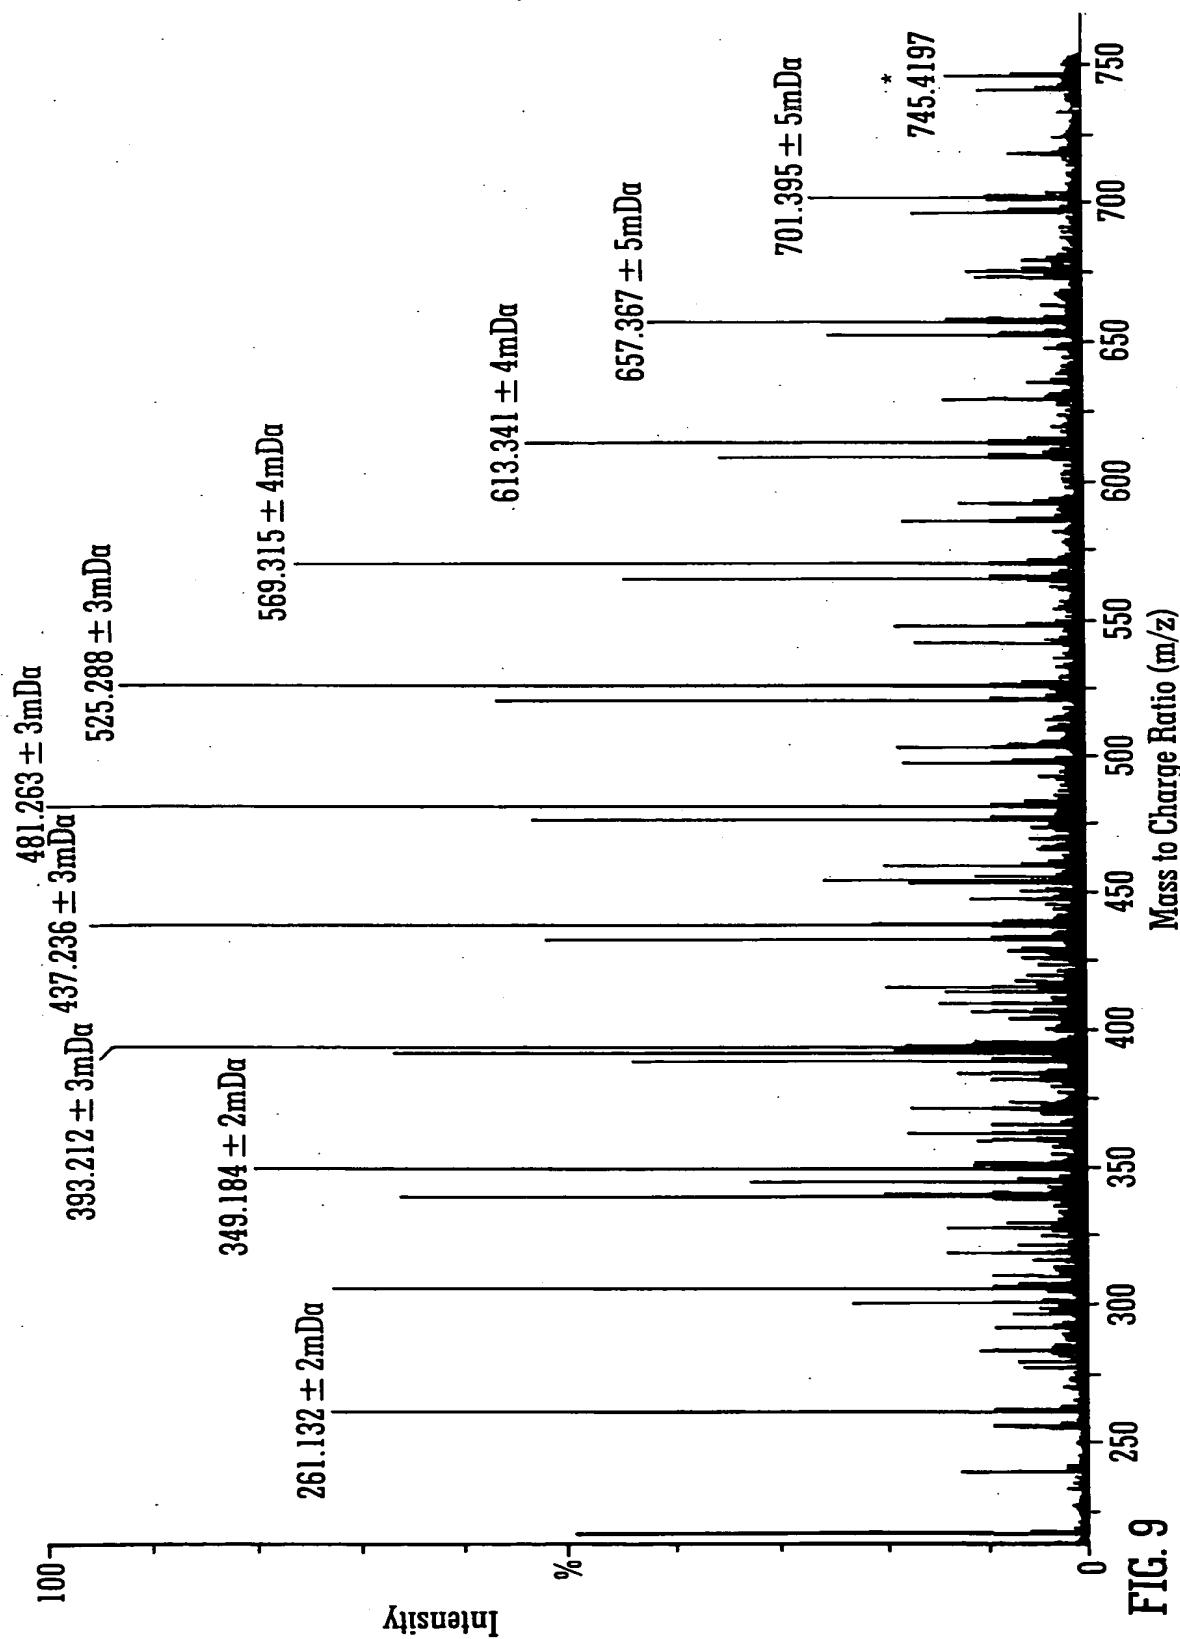


FIG. 9

BEST AVAILABLE COPY